



Disinfection fluid Monitor Series

Online Dissolved Ozone Meter T6058

Function

Online dissolved ozone meter is a microprocessor-based water quality online monitoring control instrument.

Typical Use



This instrument is widely used in online monitoring of water supply, tap water, rural drinking water, circulating water, washing film water, disinfectant water, pool water. It continuous monitoring and control water quality disinfection (ozone generator matching) and other industrial processes.

Mains Supply

85~265VAC±10%,50±1Hz, power ≤3W;
9~36VDC, power consumption≤3W;

Measuring Range


Dissolved Ozone: 0~20ppm; 0~20mg/L;
Temperature: 0~150 ℃.

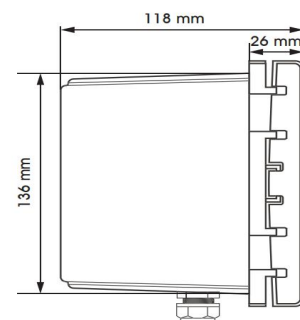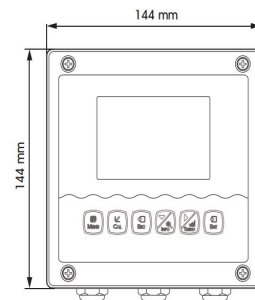

Online Dissolved Ozone Meter T6058

Features


1. Large display, standard 485 communication, with online and offline alarm, 144*144*118mm meter size, 138*138 hole size, 4.3 inch large screen display.
2. The data curve recording function is installed, the machine replaces the manual meter reading, and the query range is arbitrarily specified, so that the data is no longer lost.
3. Historical curve: The dissolved ozone measurement data can be stored automatically every 5 minutes, and the residual chlorine value can be stored continuously for a month. Provide "history curve" display and "fixed point" query function on the same screen.
4. Built-in various measurement functions, one machine with multiple functions, meeting the requirements of various measurement standards.
5. The design of the whole machine is waterproof and dustproof, and the back cover of the connection terminal is added to extend the service life in harsh environments.
6. Panel/wall/pipe installation, three options are available to meet various industrial site installation requirements.

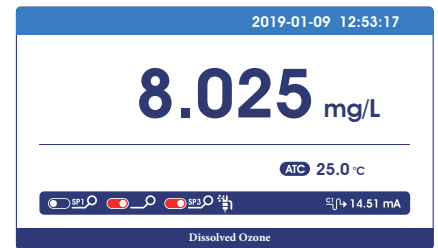

Measurement Mode



Calibration Mode

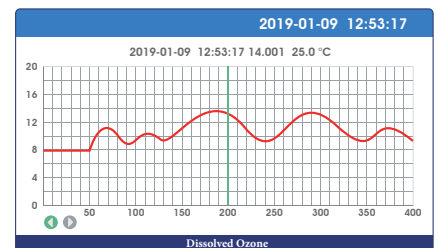

Trend Chart Display




Setting mode


Electrical connections

Electrical connection The connection between the instrument and the sensor: the power supply, output signal, relay alarm contact and the connection between the sensor and the instrument are all inside the instrument. The length of the lead wire for the fixed electrode is usually 5-10 meters, and the corresponding label or color on the sensor Insert the wire into the corresponding terminal inside the instrument and tighten it.


Instrument installation method

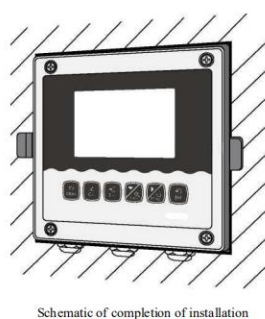

Embedded installation

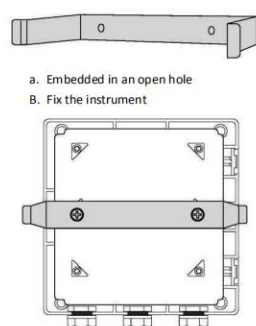

Instrument installation: Wall mounted installation

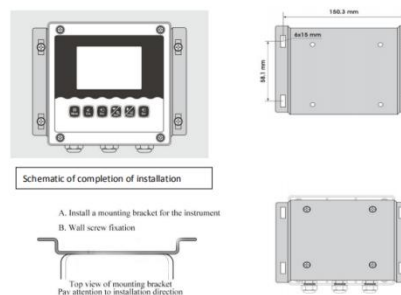

Wall mount

Technical specifications

Measurement range	0.005~20mg/L;0.005~20.00ppm
Measurement theory	Potentiometric method
Resolution	0.001mg/L;0.001ppm
Basic error	±1%F.S
Temperature	0~50.0°C
Temperature resolution	0.1°C
Temperature accuracy	±0.3°C
Temperature compensation	0~60.0°C
Temperature compensation	Manual or automatic
Electrode residual signal	<1‰
Response time	25°C < 60S; 35°C < 30S (To attain 90%)
Stability	At constant pressure and temperature, the weekly drift < 2%F•S;
Current output	Two: 4~20mA, 20~4mA, 0~20mA (load resistance < 750Ω)
Communication output	RS485 MODBUS RTU
Relay control set-points	Three: 3A 250VAC, 3A 30VDC
Optional power supply	85~265VAC, 9~36VDC, power consumption ≤ 3W
Working conditions	No strong magnetic field interference except the geomagnetic field.
Working temperature	-10~60°C
Relative humidity	≤ 90%
Waterproof rating	IP65
Weight	0.8kg
Dimensions	144×144×118mm
Installation opening size	138×138mm
Installation methods	Panel, wall mounting or pipeline

CS6530 Dissolved Ozone Sensor



Model No.	CS6530
Measurement method	Tri-electrode method
Measure material	Double liquid junction,annular liquid junction
Housing material/Dimensions	PP, Glass, 120mm* Φ 12.7mm
Waterproof grade	IP68
Measurement range	0 - 5.000 mg/L, 0 - 20.00 mg/L
Accuracy	±0.05mg/L;
Pressure resistance	≤0.3Mpa
Temperature compensation	None or Customize NTC10K
Temperature range	0-50℃
Calibration	Sample calibration
Connection methods	4 core cable
Cable length	Standard 5m cable, can be extended to 100m
Installation thread	PG13.5
Application	Tap water, disinfectant fluid, etc.